

HLL BIOTECH LIMITED, CHENNAI

INTEGRATED VACCINES COMPLEX, CHENGALPATTU

nne pharmaplan

User Requirement Specifications

Equipment/System

Sterilization Autoclave

Identification #

-

Document #

URS/SAT 03

Effective Date

04/11/2015

Revision #

00



User Requirement Specifications Sterilization - Autoclave

Block Code	Area	Identification #	Qty (Nos)	Internal Chamber Dimensions (W x H x D) in mm	Door type
R1	Measles and Rubella Bulk Block-Measles	R1-SAT-01	01	1200 x 1200 x 1800	Double door with horizontal sliding
R1	Measles and Rubella Bulk Block-Rubella	R1-SAT-02	01		
R1	Measles and Rubella Bulk Block-Media	R1-SAT-03	01		

HLL BIOTECH LIMITED, CHENNAI

INTEGRATED VACCINES COMPLEX, CHENGALPATTU

nne pharmaplan

User Requirement Specifications

Equipment/System

Sterilization Autoclave

Identification #

-

Document #

URS/SAT 03

Effective Date

04/11/2015

Revision #

00




Table of Contents

1.0	APPROVAL SIGNATURE	4
2.0	EQUIPMENT DESCRIPTION.....	5
3.0	PROCESS DESCRIPTION	7
3.1	INPUT & CHARGING METHOD	7
3.2	BRIEF PROCESS STEPS	7
3.3	OUTPUT & DISCHARGING METHOD	8
4.0	PRODUCTIVITY REQUIREMENT.....	8
4.1	DESIRED/ SUGGESTED CAPACITY	8
4.2	STANDARD BATCH SIZE	8
4.3	CHANGE OVER TIME.....	8
4.4	OTHER PRODUCTIVITY REQUIREMENT	8
5.0	CONTAINMENT	8
6.0	GMP REQUIREMENTS	8
6.1	PROCESS CONTROL.....	8
6.2	FAILURE MODE DETECTION.....	10
6.3	IN -PROCESS CONTROL	11
6.4	LEVEL OF INSTRUMENTATION	11
6.5	BATCH DATA DISPLAY AND RECORD PRINTING	12
6.6	GMP REQUIREMENTS (OTHERS).....	13
6.7	SPECIFIC REQUIREMENTS.....	14
7.0	CONSTRAINTS.....	16
7.1	EQUIPMENT LOCATION AND AVAILABLE SPACE	16
7.2	AVAILABLE UTILITY	16
8.0	ABBREVIATION.....	17
9.0	REVISION INDEX.....	17

HLL BIOTECH LIMITED, CHENNAI

INTEGRATED VACCINES COMPLEX, CHENGALPATTU

nne pharmanplan	User Requirement Specifications				 HLL BIOTECH LIMITED (a subsidiary of HLL Vaccine Research in Government of India)
	Equipment/System	Sterilization Autoclave			
	Identification #	-	Document #	URS/SAT 03	
	Effective Date	04/11/2015	Revision #	00	

URS Annexure List

URS Annex No.	Detail
1.	Layouts showing location of the Sterilization – Autoclaves (SAT)
2.	List of Preferred Make of Components
3.	List of critical items to be supplied along with the package

HLL BIOTECH LIMITED, CHENNAI

INTEGRATED VACCINES COMPLEX, CHENGALPATTU

nne pharmaplan

User Requirement Specifications

Equipment/System Sterilization Autoclave

Identification #

-

Document #

URS/SAT 03

Effective Date

04/11/2015

Revision #

00



1.0 APPROVAL SIGNATURE

This document is prepared by the Process, Validation and GMP Compliance team of "NNE Pharmaplan India" for the project "Integrated Vaccines Complex, Chengalpattu, Chennai" (project number: 120310) of HLL BIOTECH LIMITED (Chennai) under the authority of their Project Manager. Hence, this document before being effective should be reviewed by HBL user/s and project/ engineering team, approved by team lead of user department and QA and authorized by the appropriate Project Authority.

NNE Pharmaplan			
Name	Designation	Signature	Date
Prepared by			
Mr. Yogesha M J	Process Engineer	<i>Yogesha M.J.</i>	02/11/2015
Checked by			
Mr. Pulkit Mittal	Sr. Process Engineer	<i>Pulkit Mittal</i>	02/11/2015
Approved by			
Mr. Vikas Katial	GM-Projects (SME) & Head COC Vaccines	<i>Vikas Katial</i>	02/11/2015


HLL Biotech Limited			
Name	Designation	Signature	Date
Reviewed by			
User Department - (Measles & Rubella) <i>K. RADHAKRISHNAN</i>	<i>Dir. PRODUCTION</i>	<i>K. Radhakrishnan</i>	03/11/2015
QA Department <i>K. SREEKANTH</i>	ASSISTANT MANAGER	<i>K. Sreekanth</i>	03/11/2015
Project/ Engineering Department <i>A. Anirudh</i>	Manager	<i>A. Anirudh</i>	03/11/2015
Approved By			
Head of Department (Measles & Rubella) <i>D. R. Srinivasan</i>	<i>DP</i>	<i>D. R. Srinivasan</i>	03/11/2015
Head of Department (Quality Assurance) <i>D. Srinivasan</i>	<i>QA</i>	<i>D. Srinivasan</i>	04/11/2015
Authorized by			
CEO-HBL <i>Raman K. Ramachandran</i>	CEO	<i>Raman K. Ramachandran</i>	04/11/2015

HLL BIOTECH LIMITED, CHENNAI

INTEGRATED VACCINES COMPLEX, CHENGALPATTU

nne pharmaplan®

User Requirement Specifications			
Equipment/System	Sterilization Autoclave		
Identification #	-	Document #	URS/SAT 03
Effective Date	04/11/2015	Revision #	00



HLL BIOTECH LIMITED

Subsidiary of HLL Biotech Limited

10th Floor, 10th Main Road, Chengalpattu

2.0 EQUIPMENT DESCRIPTION

Autoclave for sterilization should have following main features:

- Operation programs for liquid, solid and porous materials

Package Unit (PU) including the following:

- Sterilizer chamber
- Supporting structure
- Integrated vacuum system
- Filters for process air and for exhaust air
- Piping (valves, safety devices, filters, steam traps, pipes, fittings, etc.)
- Sanitary type pressure reducing valve in pure steam inlet (for regulating the pure steam inlet pressure to the autoclave chamber as the header pressure is more than 3.0 kg/cm²).
- All mating flanges/fittings, gaskets, bolts and screws for utility supplies, returns and drain
- Instrumentation
- The unit should be direct steam heated as well as jacket steam heated and designed for full vacuum.
- Control system with printer for batch report and color trend printing
- Bio shield to seal the sterile and non-sterile areas
- One flexible probe to be provided to perform product cycle development and auto sequence to be provided.
- Small valve for steam pulsing should be provided in the steam sterilizer design

Design, function and control of the units has to be **GMP compliant**

All points of the IRS except the below mentioned would be applicable for the equipment

- 4.1.11, 4.1.13, 4.1.17
- **Sec 5.1 Table 2**
 - SI.NO 5 CE Conformity,
 - SI.NO 7 ANSI/NSF 49-2008,
 - SI.NO 8 ISO 14664
 - SI.NO 9 ISO 8362

HLL BIOTECH LIMITED, CHENNAI

INTEGRATED VACCINES COMPLEX, CHENGALPATTU

nne pharmanplan

User Requirement Specifications

Equipment/System

Sterilization Autoclave

Identification #

-

Document #

URS/SAT 03

Effective Date

04/11/2015

Revision #

00



Note:

i.	This Technical Specification is the basis for an inquiry to a vendor and therefore the basis for the vendor's proposal.
ii.	The vendor is asked to state in "REMARKS" column with "yes" if the described requirement will be completely fulfilled and with "no" in case the requirement will not or cannot be fulfilled with the proposed equipment. In case of an deviation a comment must be inserted or enclosed as a separate annexure by referring to the respective URS specification number.
iii.	The vendor must clearly comment each item of the Technical Specification. The comments must be in English language. If extra cost for necessary options becomes necessary the item must be clearly stated.
iv.	In case that the requirement includes a question or request or information from the vendor, the answer / information should be stated in the "REMARKS" column.
v.	The final version of this document including the vendor's comments will become basis of a potential purchase order or contract.
vi.	The Technical Specification serves to define a summary of all vendor's requirements concerning scope of delivery and services.
vii.	The vendor is responsible for technically unobjectionable function of the equipment. This TS is not intended to dictate a technical design to the vendor. If agreed upon with the vendor, the vendor can apply his practically proven design.
viii.	<p>Special Instruction</p> <p>a. If no comments against any specification should be considered as "NO" and</p> <p>b. If there is no reply / comments against the complete URS by the vendor then it should be treated as unresponsive / technically non-compliant and rejected.</p>
ix.	All the instruments and controls mentioned in the URS(s) are expected to be standard supply and part of your standard equipment model. In case of any deviation or redundancy or additional scope of supply is noticed, vendor is required to obtain clarification from HBL before submitting the quotes.
x.	The makes requested are standard international makes. In case of any deviation, vendor to seek clarification from HBL before submitting the offers.
xi.	Refer document Installation Requirement Specification and Specific Instructions with URS; NPI_120310_IRS_S1_01
xii.	Refer Tender document with URS: NPI-120310-EQP-S1-TD-15

HLL BIOTECH LIMITED, CHENNAI

INTEGRATED VACCINES COMPLEX, CHENGALPATTU

nne pharmanplan

User Requirement Specifications

Equipment/System

Sterilization Autoclave

Identification #

Document #

URS/SAT 03

Effective Date

09/11/2015

Revision #

00



Specifications

Remarks

3. Heating (Steaming)
4. Hold period (Sterilization)
5. Post vacuum
6. Drying
7. Unloading

3.3 Output & Discharging method

- 3.3.1 All sterilized articles will be unloaded from the unloading side by using unloading Trolley.
- 3.3.2 Chamber Carriage will be taken out and articles will be unloaded from the carriage.
- 3.3.3 All condensates and liquids should lead to common drain.

4.0 PRODUCTIVITY REQUIREMENT

4.1 Desired/ suggested capacity

Sterilization Autoclave (SAT):

Sl. No	Area	Identification #	Internal Chamber Dimensions (W x H x D) in mm	Qty (Nos)
1	Measles and Rubella Bulk Block- Measles	R1-SAT-01	1200 x 1200 x 1800	01
2	Measles and Rubella Bulk Block- Rubella	R1-SAT-02	1200 x 1200 x 1800	01
3	Measles and Rubella Bulk Block- Media	R1-SAT-03	1200 x 1200 x 1800	01

Chamber total volume: Vendor to specify

4.2 Standard batch size

Not applicable

4.3 Change Over Time

Not applicable

4.4 Other Productivity Requirement

Total sterilization cycle must not to exceed 2 hours.

5.0 CONTAINMENT

Not applicable

6.0 GMP REQUIREMENTS

6.1 Process control

- 6.1.1 The equipment must operate and control the following process cycle:

HLL BIOTECH LIMITED, CHENNAI

INTEGRATED VACCINES COMPLEX, CHENGALPATTU

nne pharmaplan

User Requirement Specifications

Equipment/System

Sterilization Autoclave

Identification #

-

Document #

URS/SAT 03

Effective Date

04/11/2015

Revision #

00



Specifications

Remarks

- Vacuum leak test cycle (As per HTM 2010)

- Bowie Dick cycle (17 min at 121 °C and 3.5 min at 135 °C)

- Standard sterilization cycle (loading → steaming → hold period → slow/fast exhaust (for liquid cycle, the exhaust will be slow)

- Standard cycle 1- Liquid (123 °C)

- Standard cycle 2 -Fabric (134 °C)

- High-pressure high vacuum sterilization cycle (loading → steam/vacuum pulsing → heat up → hold period → exhaust → vacuum drying → vacuum break by sterile air.

6.1.2 For the above processes following are the critical process parameters which must be controlled by the equipment

- Pre vacuum

- Pre pressure

- No. of Pre pulses

- Heat up

- Heat up hold

- Heat up control band

- Sterilization hold temperature

- Sterilization hold time

- Temperature control band

- Overshoot temperature

- Sterilization stop temperature

- Sterilization reset temperature

- Post vacuum start pressure

- Post vacuum

- Post vacuum hold time

- Vacuum break

HLL BIOTECH LIMITED, CHENNAI

INTEGRATED VACCINES COMPLEX, CHENGALPATTU

nne pharmaplan

User Requirement Specifications

Equipment/System

Sterilization Autoclave

Identification #

-

Document #

URS/SAT 03

Effective Date

04/11/2015

Revision #

00



Specifications

Remarks

- No of post vacuum
- Exhaust ON
- Exhaust OFF
- Process end pressure
- Chamber pressure high and low
- Jacket pressure high and low
- Too long time for pre vacuum
- Too long time for heat up

6.2 Failure mode detection

6.2.1 The Autoclave should be capable to detect the following failure, notify the operator with alarm and shutdown the process:

6.2.1.1 If chamber vacuum leak test is failed

6.2.1.2 If the chamber temperature overshoots

6.2.1.3 If chamber temperature falls below specified level & the timer stops counting

6.2.1.4 If chamber temperature falls further below specified level & the timer resets previously counted time

6.2.1.5 If chamber pressure is greater than the set value

6.2.1.6 Too long time for heat up

6.2.1.7 Too long time for pre vacuum

6.2.1.8 Too long time for post vacuum

6.2.1.9 If vacuum pump trips

6.2.1.10 Door pre-condition fails

6.2.1.11 Failure in utility supply

a) Compressed air pressure low

b) Plant steam pressure low

c) Pure steam pressure low

d) Softened water pressure low

6.2.1.12 Failure in data communication

HLL BIOTECH LIMITED, CHENNAI

INTEGRATED VACCINES COMPLEX, CHENGALPATTU

nne pharmaplan

User Requirement Specifications

Equipment/System Sterilization Autoclave

Identification #

-

Document #

URS/SAT 03

Effective Date

04/11/2015

Revision #

00



Specifications

Remarks

6.2.1.13 Vendor should propose detailed list of alarms and interlocks in Functional specifications. The alarms and interlocks list should be finalized with the final user during discussion of detailed engineering design of the equipment

6.2.1.14 Emergency stop activated

6.2.1.15 Power / UPS failure

6.2.1.16 End of cycle and door opening after end of cycle need notification to operator for procedural control

6.3 In -Process control

Manual diaphragm valves should be provided for sampling the pure steam & chamber condensate.
All necessary ports for steam quality testing as per EN 285 should be incorporated.

6.4 Level of instrumentation

Sufficient and suitable instrumentation for the process, safety and productivity control as indicated in the following table:

Type of control	Purpose/ Observation	Operation range	Desired Least Count	Extent of Instrumentation			
				Indication	Alarm	Control	Recording
Temperature (multipoint), min 6 Nos.	Chamber temperature	0°C to + 150°C	0.1°C	Y	Y	N	Y
Temperature	Chamber condensate drain	0°C to + 150°C	0.1°C	Y	Y	Y	Y
Temperature	Jacket temperature	0°C to + 150°C	0.1°C	Y	Y	Y	Y
Temperature	Air leak	0°C to + 150°C	0.1°C	Y	Y	Y	Y
Time	Sterilization time	On real time basis	1 Sec	Y	Y	Y	Y
Pressure	Chamber pressure and vacuum	Full vacuum to 2000 mbar	1.0 mbar	Y	Y	Y	Y
Pressure	Jacket pressure	0 to 5.0 bar	0.1 bar	Y	Y	Y	N
Pressure	Pressure across the sterilizing grade	0 to 2000 mbar	1.0 mbar	Y	N	N	N

HLL BIOTECH LIMITED, CHENNAI

INTEGRATED VACCINES COMPLEX, CHENGALPATTU

nne pharmaplan®

User Requirement Specifications

Equipment/System Sterilization Autoclave

Identification #

-

Document #

URS/SAT 03

Effective Date

04/11/2015

Revision #

00



Specifications

Remarks

for connecting disposable capsule filter to be provided at the unloading side.

6.6.6 Provision for air leak probe as per HTM 2010

6.6.7 Jacket to be provided with steam trap.

6.6.8 Sampling valve in the steam inlet line for collection of steam sample.

6.6.9 For easy & safety operation vendor should provide the condenser in the steam sample valve outlet

6.6.10 Sampling valve in the condensate drain line for collection of condensate sample.

6.6.11 Vendor to give code numbers for each component. Name tag of the components should be of SS plates & it should be tied with SS rope.

6.6.12 Equipment, valves, and instrumentation should be uniquely identified in accordance with a standard numbering and location system. The system will be agreed between Vendor and Client at the time of order.

6.6.13 SS panel to be flushed appropriately to the wall /ceiling/floor/LAF accordingly to avoid any dead space along with the coving on all the sides and corners.

6.6.14 All valves and instruments are to be physically tagged /labeled with their equipment numbers.

6.6.15 All the valves with in the sterile boundary must be of diaphragm valve.

6.7 Specific requirements

6.7.1 Indication of chamber pressure by pressure gauge and visual LED for door open/ close mounted on loading side and unloading side

6.7.2 Door type for autoclaves as follows :

Area	Identification #	Door Type
Measles and Rubella Bulk Block- Measles	R1-SAT-01	Double door with horizontal sliding
Measles and Rubella Bulk Block- Rubella	R1-SAT-02	
Measles and Rubella Bulk Block- Media	R1-SAT-03	

6.7.3 Fully automatic PLC based operation.

6.7.4 Control Panel should be placed in the loading side of the autoclave.

6.7.5 Arrangement of alternative power supply (UPS) to control and monitoring system.

File Name

NPI_120310_EQP_URS_SAT 03

Start Date

26-10-2015

Page No.

Page 14 of 21

HLL BIOTECH LIMITED, CHENNAI

INTEGRATED VACCINES COMPLEX, CHENGALPATTU

HBL HLL BIOTECH LIMITED A Unit of HLL Life Sciences Limited A Division of HLL Group	User Requirement Specifications			
	Equipment/System	Sterilization Autoclave		
	Identification #	-	Document #	URS/SAT 03
	Effective Date	06/11/2015	Revision #	00

Specifications	Remarks
6.7.6 All utility points will be provided nearer to the equipment. Hooking up of the equipment to the nearest utility points will be in the vendor's scope.	
6.7.7 Pressure relief valve should be provided for safety purposes	
6.7.8 Automatic F ₀ value calculation for each temperature monitoring port	
6.7.9 The chamber floor should be on the same plane with the floor of the trolley, so that the loading carriage can directly be moved into the chamber	
6.7.10 The trolley should carry two different carriages at a time and the chamber should also accommodate two carriages.	
6.7.11 Sterilization Chamber: The chamber should be rectangular, with smooth and rounded corners. The chamber should be designed as per ASME pressure vessel code. The chamber should be made of SS316L with surface roughness less than 0.6µm. The chamber should be re-inforced with an SS 304 jacket. The sterilizer support frame for the entire structure should be made of SS 304. The sterilizer should be able to reach and maintain sterilization temperature of 121°C- 134°C. The temperature should be settable parameter.	
6.7.12 Chamber Doors: Steam Sterilizers should have sliding double door with automatic closing and opening. The door should be made of SS 316L with internal surface roughness less than 0.6µm. The door gaskets should be made of high temperature resistant silicone rubber with rounded corners	
6.7.13 Door Safety The following door safety features should be provided for operator safety: <ul style="list-style-type: none"> • Door interlocking to prevent simultaneous opening of both the doors. • Door process lock to prevent opening of doors when the process is ON • Door obstructive sensor to be provided 	
6.7.14 FAT/SAT the following need to be demonstrated : a. All probes to reach 121 °C within 30 sec of the first probe for above 800L capacity chamber and 15 sec for below 800 L Chamber capacity. b. Temperature differences between any two probes should not be more than 1 °C during hold time. c. Temperature Recorders should have accuracy of at least 1% over range 50 °C to 150 °C. d. Pressure recorders should have accuracy of ±1.6 % over the range of 1 bar to 3 bar. e. Pressure recorders should have an accuracy of at least 0.01 bar. f. Temperature variation during sterilization hold time should not be more than 1 °C	

HLL BIOTECH LIMITED, CHENNAI

INTEGRATED VACCINES COMPLEX, CHENGALPATTU

nne pharmaplan

User Requirement Specifications

Equipment/System	Sterilization Autoclave		
Identification #	-	Document #	URS/SAT 03
Effective Date	04/11/2015	Revision #	00



Specifications

Remarks

7.0 CONSTRAINTS

7.1 Equipment location and available space

This equipment will be installed in the **Measles and Rubella Bulk Block of Integrated Vaccines Complex, at Chengalpattu**

The equipment location is indicated in the relevant block of the layout enclosed as URS Annex-1.

Block Name	Identification #	Loading Room No.	Unloading Room No.
Measles and Rubella Bulk Block- Measles	R1-SAT-01	R1G031	R1G042
Measles and Rubella Bulk Block- Rubella	R1-SAT-02	R1G075	R1G102
Measles and Rubella Bulk Block- Media	R1-SAT-03	R1G029	R1G033

7.2 Available Utility

- Electricity: _____ (Report Requirement)
- Pure steam: 3 bar (Report Requirement)
- Plant Steam: 3-3.5 bar (Report Requirement)
- Chilled water/ soft water : Supply: 6-7degC, Return: 11-12deg C (or depends on process) / Amb (Report Requirement)
- Compressed air : 8-10 bar g (Report Requirement)

Note:

1. Vendor to provide Vacuum system, Pressure reducing valves and Pressure gauges along with the equipment as per equipment utility requirements.
2. Vendor to provide the all utility consumptions in details for the equipment in the technical bid.
3. Control panel, HMI & printer should be placed in loading side of the autoclave.

HLL BIOTECH LIMITED, CHENNAI

INTEGRATED VACCINES COMPLEX, CHENGALPATTU

nne pharmaplan

User Requirement Specifications

Equipment/System Sterilization Autoclave

Identification #

-

Document #

URS/SAT 03

Effective Date

04/11/2015

Revision #

00



8.0 ABBREVIATION

List of abbreviations

HTM	Health Technical Memorandum
ISO	International Standard Organization
HBL	HLL Biotech Limited
LAF	Laminar Air Flow
PLC	Programmable Logic Controller
NNE	Novo Nordisk Engineering
SAT	Sterilisation Autoclave
SS	Stainless steel
URS	Users Requirement Specification
HMI	Human Machine Interface

9.0 REVISION INDEX

Revision	Date	Reason for revision
00	27-10-2015	First Draft for Client's Review

HLL BIOTECH LIMITED, CHENNAI

INTEGRATED VACCINES COMPLEX, CHENGALPATTU

nne pharmaplan

User Requirement Specifications

Equipment/System Sterilization Autoclave

Identification #

Document #

URS/SAT 03

Effective Date

09/11/2015


Revision #

00




URS Annexure-1: Layouts showing location of the Sterilization – Autoclaves (SAT)

1. R1-SAT 01

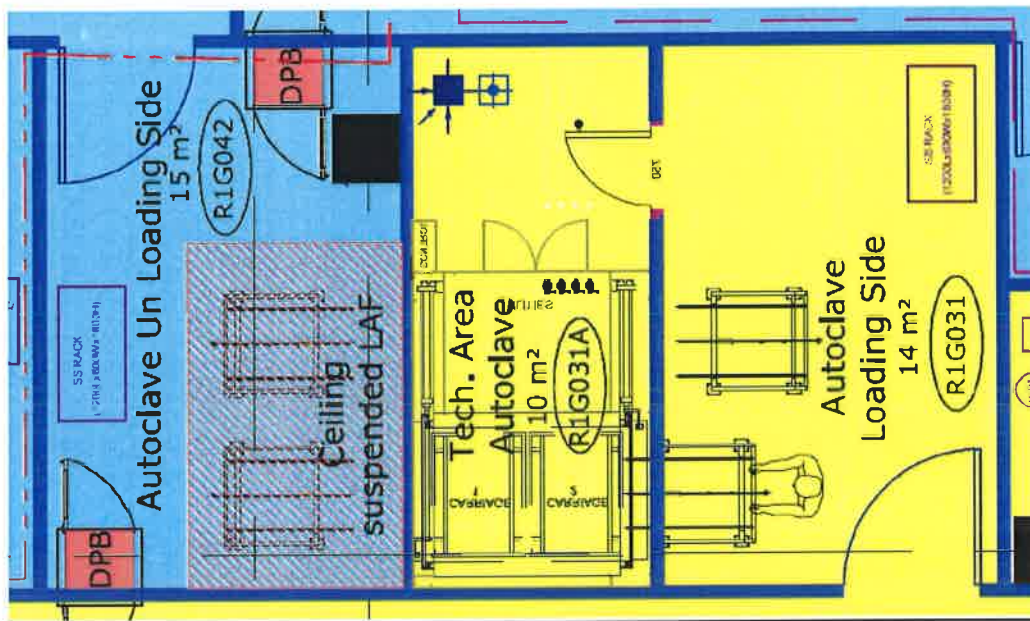

2. R1-SAT 02

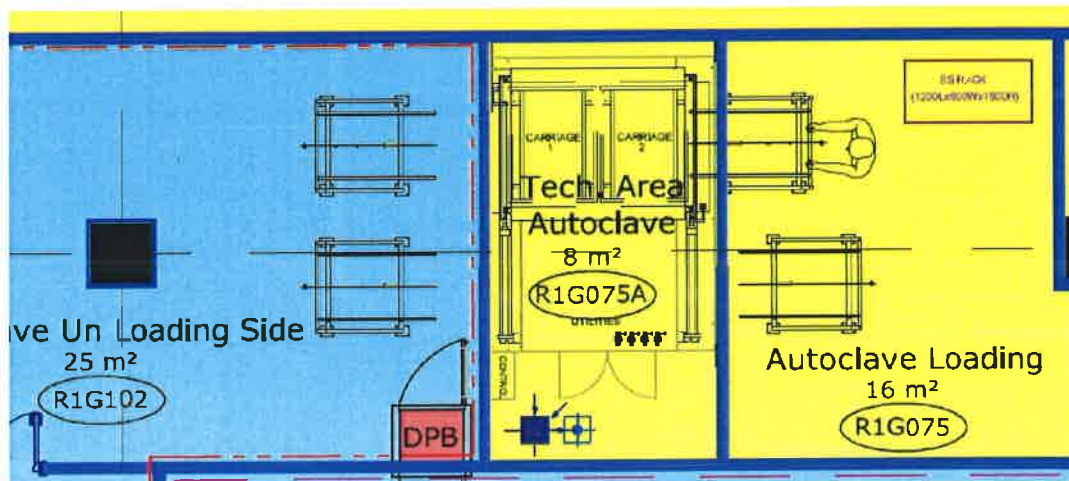

HLL BIOTECH LIMITED, CHENNAI

INTEGRATED VACCINES COMPLEX, CHENGALPATTU

nne pharmaplan®

User Requirement Specifications

Equipment/System Sterilization Autoclave

Identification #

-

Document #

URS/SAT 03

Effective Date


04/11/2015

Revision #

00



3. R1-SAT 03

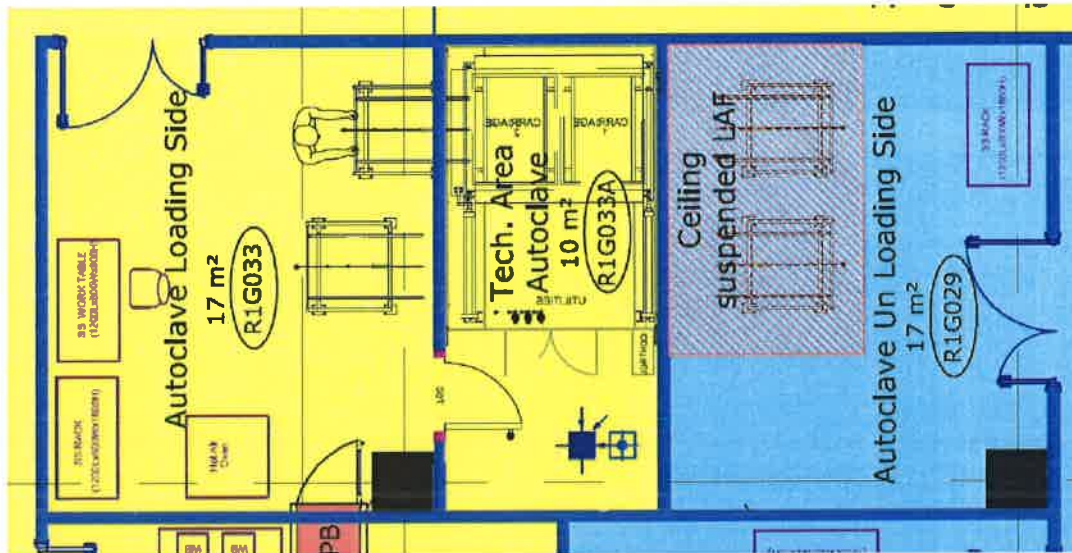

HLL BIOTECH LIMITED, CHENNAI

INTEGRATED VACCINES COMPLEX, CHENGALPATTU

nne pharmaplan

User Requirement Specifications

Equipment/System Sterilization Autoclave

Identification #

Document #

URS/SAT 03

Effective Date

04/11/2015

Revision #

00



URS Annexure 2: List of Preferred Make of Components

SL.NO	DESCRIPTION	MAKE
A	INSTRUMENTATION	
1.	PLC/HMI	Allen Bradley/ Siemens
2.	Operator Interface	Allen Bradley/ Siemens
3.	Temperature transmitter	Radix/ Yokogawa/ Emerson
4.	Pressure transmitter	Siemens/ Jumo/ Wika
5.	RTD sensors	Radix/ Wika/ Waaree Instruments
6.	Temperature indicator controller	Radix/ Wika/ Waaree Instruments
7.	Printer	Epson/ HP/ Canon
8.	DC source	Shavision/ Yokogawa/ Emerson
9.	Photocell sensor	P & F/ Optex/ Metler
B	MECHANICAL	
1.	Automatic Angle Valve	Gemu / ITT / SED
2.	Manual Ball Valve	President/ Modentic
3.	Needle Valve	President/ Modentic
4.	Safety Valve	Teleflo/Herose/ Ciprani Harrison
5.	Pressure Reducing Valve	Klinger/ Forbes Marshall/ Armstrong International
6.	Sanitary PRV	Jordon / Forbes Marshall/ Sarco
7.	Non Return Valve	Leader/ Modentic/ Alfa Laval
8.	Pressure Gauges	Forbes Marshall/ Wika/ Waaree Instruments
9.	Pressure & Vacuum Switch	Orion/ Wika/ Emerson/ Danfos
10.	Steam Trap	Spirax / ITT
11.	Vacuum Break Filter	Sartorius/ Pall/ Millipore
12.	Vacuum Pump	Newgenre / PPI
C	PNEUMATIC	
1.	Pneumatic door operating cylinder	Janatics/Rotex
2.	Solenoid valves for door	Janatics/ Festo
3.	Solenoid valves for Gasket	Festo/ Danfos / Janatics
4.	Solenoid valves for Process Valves	Janatics/ Festo
5.	Filter Regulator Lubricator	Janatics/ Festo
6.	Diaphragm Valve (Sterile side)	GEMU / ITT / SED
D	ELECTRICAL	
1.	Limit switches	Bohmen / Siemens/ Emersen
2.	Switch gear and Relays	Siemens/ L&T/ Schneider
3.	Miniature circuit breaker	Siemens/ Havells / Legrand
4.	Rotary switch	L&T/ Siemens/ Schneider
5.	Indication lamps	Technik / Mimic/ Schneider

HLL BIOTECH LIMITED, CHENNAI

INTEGRATED VACCINES COMPLEX, CHENGALPATTU

nne pharmaplan

User Requirement Specifications

Equipment/System

Sterilization Autoclave

Identification #

Document #

URS/SAT 03

Effective Date

04/11/2015

Revision #

00

HBL

HLL BIOTECH LIMITED

(a subsidiary of HLL Life Sciences Limited)

(A Division of HLL Group)

URS Annexure 3: List of critical items to be supplied along with the package

SL.NO	DESCRIPTION	NO. OF QUANTITY
1.	Door gasket	2 set for each size
2.	Pressure switch	5 No.s
3.	Vacuum switch	5 No.s
4.	Pressure Gauge	5 No.s
5.	Compound Gauge	5 No.s
6.	Coil for Solenoid valves for doors	5 No.s
7.	Push buttons	10 No.s
8.	Coil for Solenoid valves for process	5 No.s
9.	Rotary Switch	4 No.s
10.	Indication bulb sets	10 No.s
11.	Temperature transmitter	4 Nos